




Certificate of Analysis

10 SEPTEMBER 2023
 HKSHTVC300 / MIT / F98F4

CLIENT:	HulkHogan	SAMPLE SET:	159650
Sample Type:	Liquid	Date Acquired:	09/06/2023
Sample Weight:	2mL	Acquisition Method:	MIT-EVO_R2023-01
Dilution:	0.1	Testing ID:	GRD-MIT_154293.D
Vial:	Vial 2	Date Processed:	09/10/2023
Injection Volume:	5.0 µl	Run Time:	27 min
Prepped By:	Sarah T.	Calibration ID:	20230105

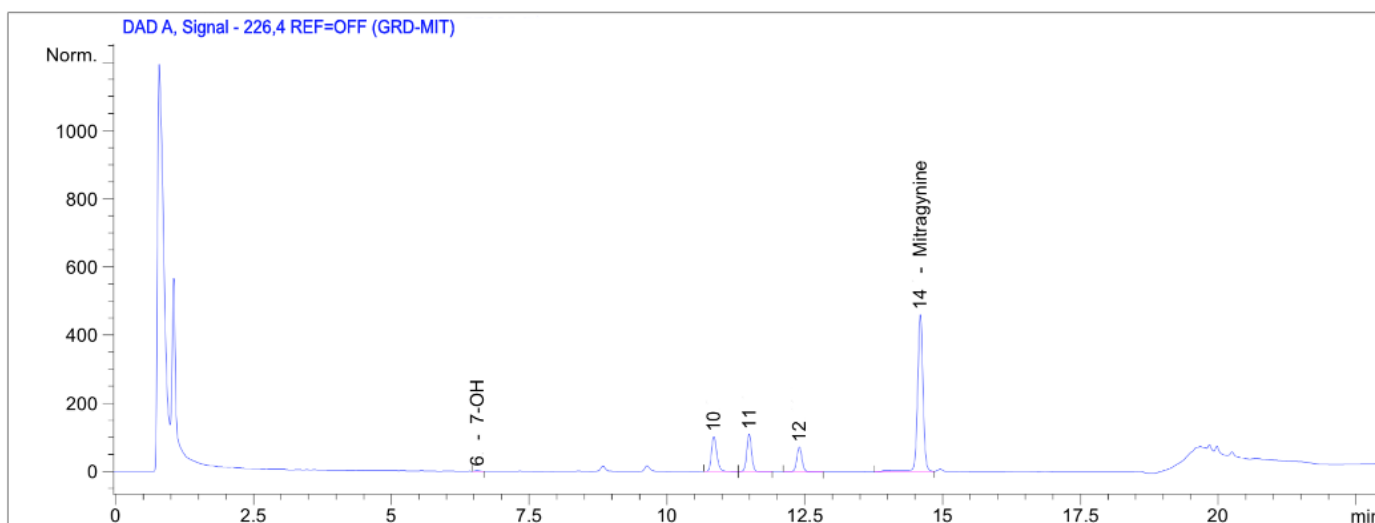

#	Analyte	RT (min)	Area (mAU*s)	Amt (µg/mL)	Alkaloid	Total %
1	Mitragynine	14	4078	197	C ₂₃ H ₃₀ N ₂ O ₄	.46
2	7-Hydroxymitragynine	6	N/D	N/D	C ₂₃ H ₃₀ N ₂ O ₅	N/D
3	Paynantheine	10	122	6	C ₂₃ H ₂₈ N ₂ O ₄	0.01
4	Speciogynine	11	422	20	C ₂₃ H ₃₀ N ₂ O ₄	0.02
5	Speciociliatine	12	260	13	C ₂₃ H ₃₀ N ₂ O ₄	0.01
6						

Mitragynine Content: **5 mg/mL**

Adulterants (Y/N): **None Detected**

Identity Confirmed: **YES**

SEAL OF AUTHENTICITY

VERIFIED BY: *[Signature]*

Quality Assurance: *[Signature]*